



TEST REPORT TUCHENG

Date: Jun. 23, 2020 Date of Receipt: Jun. 04, 2020

Report No.: TFF9F110 Quantity: 1PC Page Order/Pages: (P1/4) Ref. No.: NIL

Report Title: AMBER NANOTECH CO., LTD.(U2803) Item: Mask

Address: No. 156, Keda 1st Road, Zhubei City, Hsinchu County, Taiwan


Test Items		Test Results	Test Methods
Air Exchange Pressure (Pa/cm ²)	1	29.7	EN 14683:2019 Annex C
	2	31.6	
	3	29.4	
	4	30.2	
	5	29.6	

This test report is for reference only and should not be used as a formal document.

Note: Sample description is given by the client: Ambotum High Secured Safety Nano 3D Mask

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

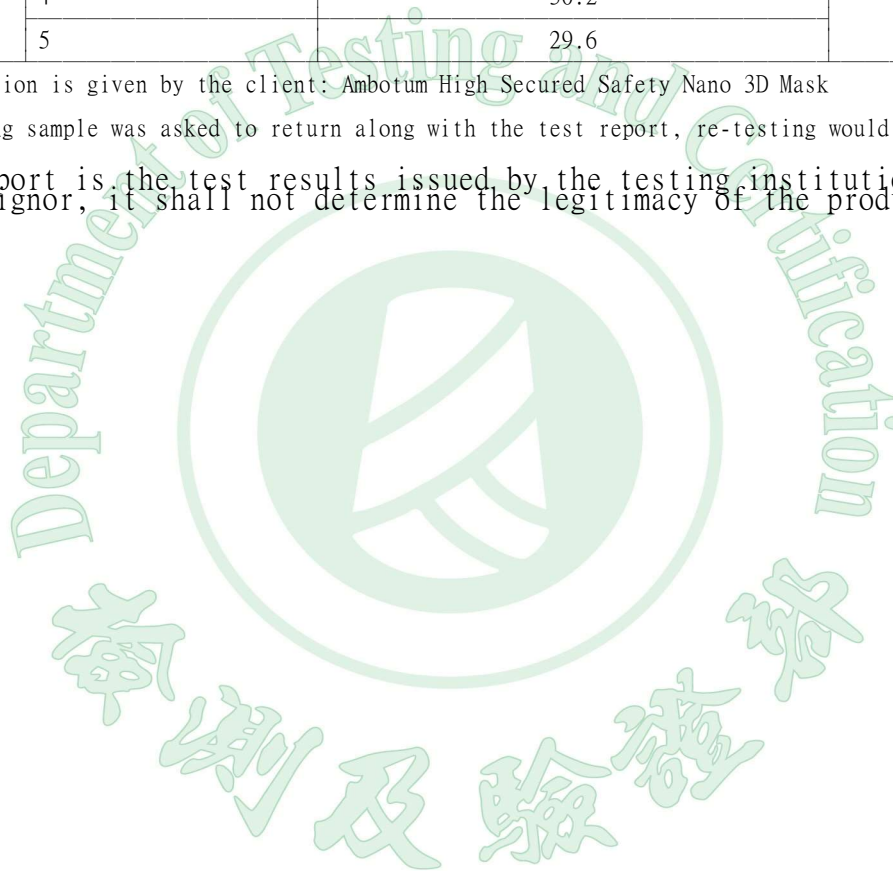

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung kao

Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839



TEST REPORT TUCHENG

Date: Jun.23,2020 Date of Receipt: Jun.04,2020

Report No.: TFF9F110 Quantity: 1PC Page Order/Pages: (P2/4) Ref. No.: NIL

Report Title: AMBER NANOTECH CO., LTD.(U2803) Item: Mask

Address: No. 156, Keda 1st Road, Zhubei City, Hsinchu County, Taiwan

Test Items		Test Results	Test Methods
Bacterial Filtration	1	99.7	EN 14683:2019 Annex B
Efficiency (BFE)(%)	2	99.6	
Staphylococcus aureus	3	99.5	
ATCC 6538	4	99.4	
	5	99.4	

This test report is for reference only and should not be used as a formal document.

Note: Control average: 2363 CFU.

Note: Mean particle size: 2.9 μm.

Note: Testing side: outside of specimen.


Note: Testing area: 36.3 cm².

Note: Flow rate : 28.3 L/min.

Note: Sample description is given by the client: Ambotum High Secured Safety Nano 3D Mask

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

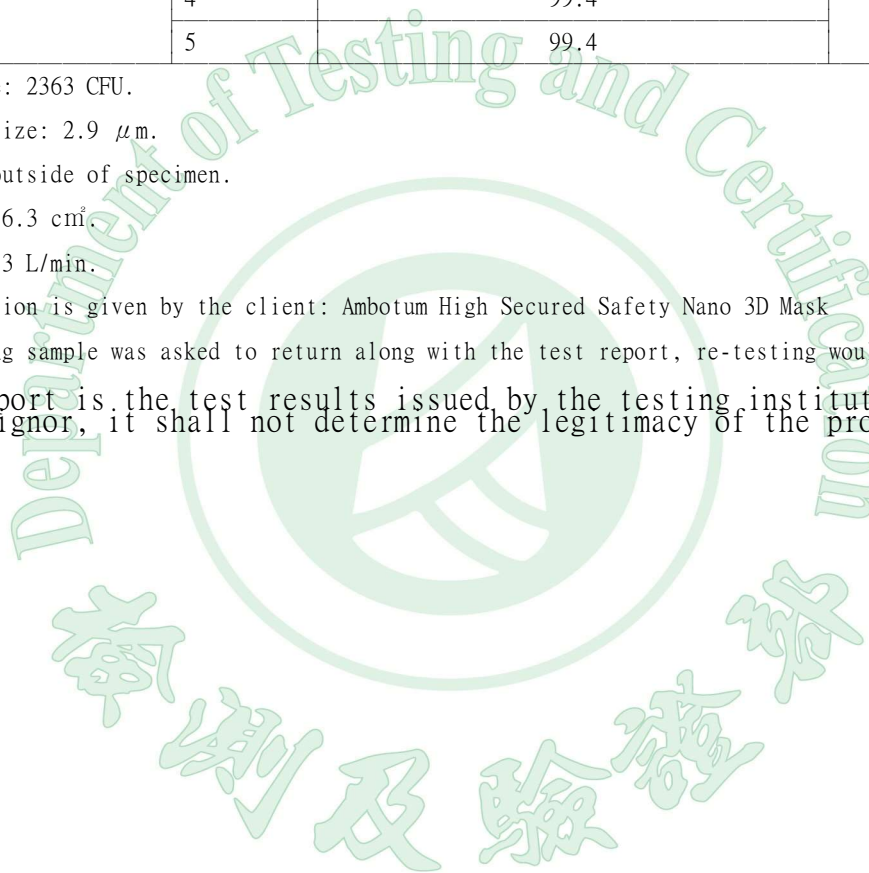

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung kao

Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108, +886-2-22689839



TEST REPORT TUCHENG

Date: Jun. 23, 2020 Date of Receipt: Jun. 04, 2020

Report No.: TFF9F110 Quantity: 1PC Page Order/Pages: (P3/4) Ref. No.: NIL

Report Title: AMBER NANOTECH CO., LTD.(U2803) Item: Mask

Address: No. 156, Keda 1st Road, Zhubei City, Hsinchu County, Taiwan


Test Items		Test Results	Test Methods
Microbial cleanliness (cfu/g)	1	7.5	EN 14683:2019
	2	11.9	EN ISO 11737-1:2018
	3	4.2	
	4	5.2	
	5	9.6	

This test report is for reference only and should not be used as a formal document.

Note: Sample description is given by the client: Ambotum High Secured Safety Nano 3D Mask

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

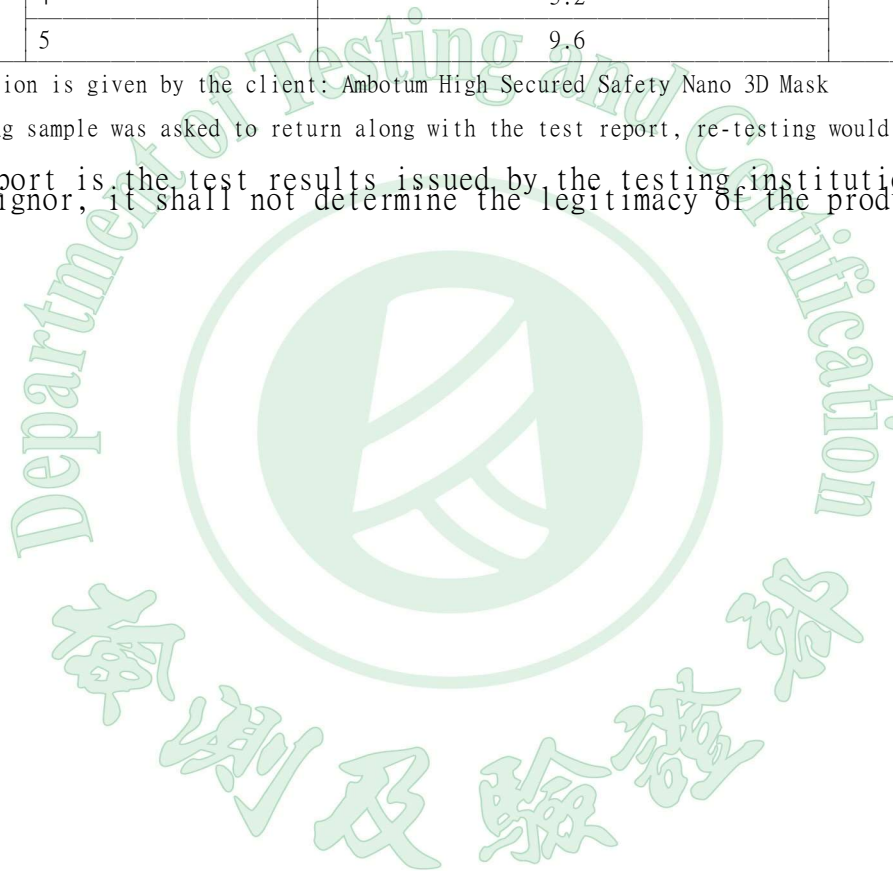

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung kao
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839



TEST REPORT TUCHENG

Date: Jun. 23, 2020 Date of Receipt: Jun. 04, 2020

Report No.: TFF9F110 Quantity: 1PC Page Order/Pages: (P4/4) Ref. No.: NIL

Report Title: AMBER NANOTECH CO., LTD.(U2803) Item: Mask

Address: No. 156, Keda 1st Road, Zhubei City, Hsinchu County, Taiwan

*This test report is for reference only
and should not be used as a formal
document.*



- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung kao
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839